

## Book Chapter

# Nanoarchitectonics of Electrically Activable Phosponium Self-Assembled Monolayers to Efficiently Kill and Tackle Bacterial Infections on Demand

Serena Carrara<sup>1†‡</sup>, Florent Rouvier<sup>2‡</sup>, Sanjana Auditto<sup>1‡</sup>, Frédéric Brunel<sup>1</sup>, Charlotte Jeanneau<sup>3</sup>, Michel Camplo<sup>1</sup>, Michelle Sergent<sup>4,5</sup>, Imad About<sup>3</sup>, Jean-Michel Bolla<sup>2\*</sup> and Jean-Manuel Raimundo<sup>1\*</sup>

<sup>1</sup>Aix-Marseille Université, CNRS, CINAM, France

<sup>2</sup>Aix-Marseille Université, INSERM, SSA, IRBA, MCT, France

<sup>3</sup>Aix-Marseille Université, CNRS, ISM, Inst Movement Sci, France

<sup>4</sup>Aix-Marseille Université, CNRS, IRD, IMBE, France

<sup>5</sup>Avignon Université, CNRS, IRD, IMBE, France

<sup>†</sup>Present address: Procter & Gamble-Brussels Innovation Center Temselaan 100, 1853 Grimbergen, Belgium.

<sup>‡</sup>These authors contributed equally to this work.

**\*Corresponding Authors:** Jean-Manuel Raimundo, Aix-Marseille Université, CNRS, CINAM, 13288 Marseille, France

Jean-Michel Bolla, Aix-Marseille Université, INSERM, SSA, IRBA, MCT, 13005 Marseille, France

Published **May 23, 2022**

This Book Chapter is a republication of an article published by Jean-Manuel Raimundo, et al. at International Journal of Molecular Sciences in February 2022. (Carrara, S.; Rouvier, F.; Auditto, S.; Brunel, F.; Jeanneau, C.; Camplo, M.; Sergent, M.; About, I.; Bolla, J.-M.; Raimundo, J.-M. Nanoarchitectonics of Electrically Activable Phosponium Self-Assembled Monolayers

to Efficiently Kill and Tackle Bacterial Infections on Demand. Int. J. Mol. Sci. 2022, 23, 2183.

<https://doi.org/10.3390/ijms23042183>)

**How to cite this book chapter:** Serena Carrara, Florent Rouvier, Sanjana Auditto, Frédéric Brunel, Charlotte Jeanneau, Michel Camplo, Michelle Sergent, Imad About, Jean-Michel Bolla, Jean-Manuel Raimundo. Nanoarchitectonics of Electrically Activable Phosphonium Self-Assembled Monolayers to Efficiently Kill and Tackle Bacterial Infections on Demand. In: Saeed Tarighi, editor. Prime Archives in Molecular Sciences: 3<sup>rd</sup> Edition. Hyderabad, India: Vide Leaf. 2022.

© The Author(s) 2022. This article is distributed under the terms of the Creative Commons Attribution 4.0 International License (<http://creativecommons.org/licenses/by/4.0/>), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

**Author Contributions:** † S. C., F. R. and S. A. contributed equally to the work. Electrochemical experiments were done by S. C. and the cellular and bacteriological tests were performed by F. R.; S.A. carried out the synthesis and substrate coatings and F. B. participated in the synthesis. The manuscript was written through contributions of all authors. All authors have read and given approval to the final version of the manuscript and gave valuable suggestions on the manuscript.

**Funding:** This work was supported by the Centre National de la Recherche Scientifique and the Ministère de l'Enseignement Supérieur et de la Recherche and was funded by a public grant overseen by the Société d'Aide au Transfert Technologique du Sud-Est (SATT-Sud Est) under the contract 780-SA-16-CNRS. S. C. and F. R. thank the SATT-Sud Est for their financial support. S. A. thanks the ministère de l'Enseignement Supérieur, de la Recherche et de l'Innovation (MESRI) for the PhD support.

**Conflict of Interest:** The authors declare no conflict of interest.

## Abstract

Prosthetic implants are widely used in dentistry and orthopedics and as a result, infections can occur causing their removal. It is therefore essential to propose methods of eradicating the bacteria that remain on the prosthesis during treatment. For this purpose, it is necessary to develop surfaces whose antibacterial activity can be controlled. Herein, we designed innovative and smart phosphonium self-assembled monolayer (SAM) interfaces that can be electrically activated on-demand for controlling bacterial contaminations on solid surfaces. Upon electroactivation with a low potential (0.2 V for 60 min., conditions determined through a *DOE*), a successful stamping out of Gram-positive and Gram-negative bacterial strains was obtained with SAM-modified titanium surfaces. Effectively killing 95% of *Staphylococcus aureus* and 90% *Klebsiella pneumoniae*. More importantly, no toxicity towards eukaryotic cells was observed which further enhances the biocompatible character of these novel surfaces for further implementation.

## Keywords

Phosphoniums; Self-Assembled Monolayers; Biocidal Effect; Electroactivation; Responsive Surfaces

## Introduction

Nowadays bacterial infections constitute a major threat to public health [1] and many experts are predicting a net increase of the mortality by 2050 caused by the rapid growth of multidrug resistant bacteria over the past decade [2,3]. To prevent this alarming scenario, it is urgent to identify new antibiotics and strategies to control bacterial proliferation. Although medical implants lead to a significant improvement in the patient's well-being and healthcare, there are several drawbacks including surgical risks during the placement or removal, implant failure and more specifically infections by pathogenic microorganisms which are important to circumvent. These implant infections are a result of a bacterial biofilm formation [4] in which bacteria are embedded into a complex matrix rendering them more


recalcitrant to conventional treatments. Implant surfaces are non-vascularized abiotic materials rendering the common strategies inappropriate and ineffective. This global issue of biofilm colonization on surfaces has driven the scientific community to develop an increasing number of novel materials possessing anti-biofilm features associated to biocidal properties [5]. The most predominant strategies to tackle the bacterial colonization are mainly based on the development of biofilm disrupting agents [6]. Other antibiofilm approaches based on the inhibition of bacterial adhesion or proliferation have also prompted strong interest [7]. Those include surfaces impregnated with antimicrobial and antiseptic hubs and cuffs [8], immunoprophylaxis [9], quorum sensing interference, impairment of staphylococci adhesion or biofilm accumulation [10], immunotherapy, enzymatic disruption, or removal of biofilm [11], immunomodulation and use of nanoparticles to deliver anti-biofilm agents [12]. Despite those treatments, biofilms can re-grow with infection relapses and prolonged treatments may develop microbes with increased resistance to biocides with cumulative side-effects of drugs that may have a substantial impact on the patient's microbiota ecology.

So far, to circumvent these drawbacks, polymers-based antifouling, or antibacterial surfaces, acting either by contact effect or continuous release of bactericidal substances (antibiotics, metal ions, peptides), have been developed to tackle bacterial adhesion and kill bacteria [13]. Furthermore, strategies that delay or prevent the continuous release of active substances have been developed [14] from bacterial infection microenvironment-responsive surfaces (pH, bacterial enzymes (lipases, hyaluronidases), etc.) [15] or light [16]. Although some of them appear promising, these coatings often lead to a gradual leaching of the biocidal substances. Therefore, these coatings are inadequate for long-term uses as infections on prostheses can occur within a relatively long time after implantation [17].

Interestingly, electrical activation has been thought to be a possible trigger for such applications [18] since it has been efficiently applied to control the binding and switching of molecules and biomolecules onto surfaces [19]. In addition, in

the late 60's [20,21], critical work on the bioelectric effect demonstrated some interesting capabilities for eliminating biofilms from colonized surfaces [22]. However, this work has been underexploited until very recently but is still in its early stages [23,24]. Moreover, we have recently demonstrated that engineered phosphoniums can be used as effective antibacterial scaffolds against bacteria from the ESKAPE group [25-27].


Thus, in line of our previous work and based on the potential benefits of the bioelectric effect we have developed novel electrically responsive surfaces possessing efficient biocidal properties made from the unique combination of phosphoniums-self-assembled monolayers onto a conductive surface such as titanium which is commonly used for implants manufacturing (Figure 1). The results emerging from this work will be helpful and used to create innovative electro-responsive surfaces that are of great interest, for example, in the design and development of smart dressings that can allow both, to monitor and eradicate microbial infections. The whole process could be controlled using mobile technologies with the possibility to have an electronic medical record and will constitute a personal point of care for patients. [28,29]

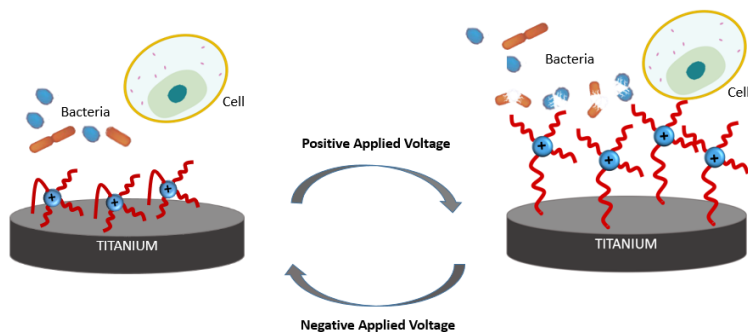

**Figure 1:** Schematic representation of electrically responsive biocidal surface based on phosphonium-self-assembled monolayers.

## Results and Discussion

The synthesis of the target trialkylphosphonium bromide derivatives 3-5 is depicted in Scheme 1 following previous published procedures [25-27]. Target compounds were readily prepared in two consecutive steps from commercially available dibromo derivatives. The first step involves a nucleophilic substitution reaction on the dibromoalkyl starting building blocks with potassium thioacetate in acetone to afford the monofunctionalized intermediates 1-2 in 65 and 74% yield respectively (See SI) [30]. The latter were subsequently treated with the appropriate trialkylphosphines using an eco-friendly method under neat conditions using a microwave irradiation at 200W (130°C) for 3 hours leading to the compounds 3-5 in 98, 55 and 43% yield respectively.

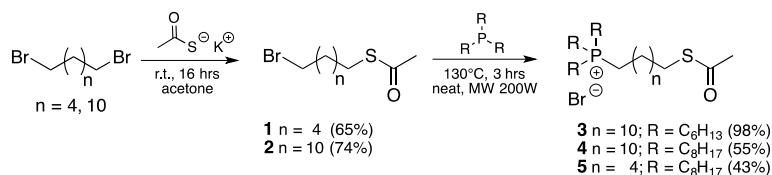


**Scheme 1:** Synthesis of the trialkylphosphoniums bromide target compounds.

All new compounds have been characterized by conventional spectroscopic analytical methods. The phosphoniums were preselected because of their biocidal efficiencies against *Staphylococcus aureus* and other Gram-positive strains from the ESKAPE group in their planktonic form according to our previous works [25-27].

Ti and its alloys are widely used in orthopedic and orthodontic implants [31] but exhibit a lack of antibacterial effectiveness activities and implants-associated rejection issues occur in the case of long term uses. Furthermore, the biocompatibility both, at the micro- and nanoscales of Ti alloys-based implants depend strongly on their composition and surface roughness [32,33] that can be improved by either a physical or chemical surface modification process. To this aim, self-assembled monolayers (SAMs) have proven to be an efficient approach to coherently

improve metallic surfaces properties including those of Ti. [34] Indeed, through careful engineering, SAMs act as dense, compact, and versatile layers that allow the modification and fine tuning of the surfaces with advanced and specific properties even on complex geometries.

The self-assembled monolayers formation onto the titanium disks was monitored by several methods including contact angle and SEM and compared with bare titanium surfaces. Contact angle of the functionalized surfaces decreased linearly with time compared to the bare surface due to the presence of the cationic phosphonium head groups suggesting the formation of a densely packed monolayer. This trait was also revealed by SEM micrographs demonstrating an increase of the surface smoothness along the time from bare titanium to the fully coated surface after 7 days (Figure 2 a-c). Furthermore, EIS measurements were used to prove the SAM formation. A solid electrolyte (agarose 1%) in water was selected to conduct these experiments. Hence, the formation of the SAM is expected to gradually modify the level of charges and dipole at the interface leading to a modification of the capacitance and resistance (Figure 2d). The real impedance  $Z_{re}$  corresponding to the resistance at the SAM/agarose interface is obtained from the EIS spectra in a Nyquist plot. In this configuration the electrode/solution interface is modeled as a simplified Randles equivalent circuit where the solution resistance and the double layer capacitance are in series. With time, the formation of the SAM steadily changes both the overall cell resistance and the capacitance since the molecular adsorption involves at least the displacement of water and ions from the interface. The resistance values were plotted against the time to generate an adsorption isotherm as depicted in Figure 2e.

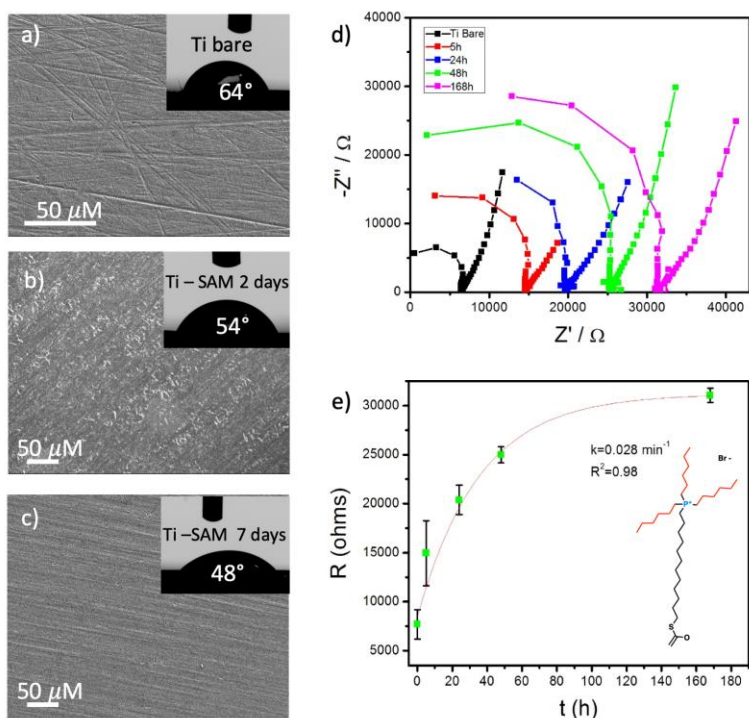


**Figure 2:** a-c) SEM micrographs of titanium bare surface, Ti-SAM of 3 after 2 days and after 7 days, respectively. Inset: contact angle images. d) Nyquist plots for Ti-SAM of 3 using agarose gel 1% as solid electrolyte. The frequency range was 0.1 Hz to 100 MHz, frequency increases from right to left, excitation signal of 25 mV peak amplitude was applied at OCP vs. Platinum wires as reference and counter electrode. e) Resistance (Ohms) vs time (hours) adsorption isotherm fit for the set of data.

SAM-modified titanium surfaces serve as models for dental implants and their antibacterial properties have been evaluated with and without electrical activation. Gram positive *Staphylococcus aureus* and Gram-negative *Klebsiella pneumoniae* were chosen as species for the proof-of-principle tests and the antibacterial effect was determined according to the percentage of the bacterial survival after each experiment. As growth controls, a glass slit was used to replace the titanium disks. Electrical activation and experiments were performed using the 3D imprinted device depicted in the Materials and Methods section (Figure 6) and were carried out under the same




conditions. An amount of  $0.5 \times 10^6$  Colony Forming Unit CFU ( $5 \mu\text{L}$  of a  $10^8$  CFU/ml bacterial suspension) was deposited on top of the agarose surface prior to being sandwiched with the bare titanium or the SAM-modified titanium surface followed by securing the whole device to ensure watertightness. At the end of the experiments, the agarose and titanium disks were shaken in MH II media to additionally count the bacterial colonies in the suspensions. Several combinations of different parameters can be tested at the same time, for instance, the nature of molecular scaffold, percentage of the SAM coverage, the type of electrochemical activation (CV/CA) and duration (30, 60, 120 min.). Due to the large number of possible experiments, a Design Of Experiment (DOE) has been set in order to obtain the best combination of parameters from a statistical plan based on a matrix calculation. The DOE offers a straightforward strategy to determine the best experimental choices that enhance the quality of the results. It helps in optimizing the parameters and gives a prompt statistical approach which is useful for an industrial application. For an overview, the dataset extrapolated from the matrix of DOE is reported in Supporting information. All the combinations described by the DOE have been tested in triplicates to obtain a weighted value and a standard deviation at the end. Among them (see ESI for more details) the most efficient SAM which gave a great statistical meaning, and the best experimental action was compound 3 with a coverage of 100% by applying a voltage of +0.2 V for 60 minutes (Figure 3). Upon these conditions (+0.2 V, 60 min.), this functionalized surface, in contact with *S. aureus*, displayed a remarkable biocidal efficiency up to 95% compared to the untreated surface used as a reference. Encouraged by these results, experiments on Gram-negative bacteria have also been investigated by using the optimal conditions found for Gram-positive bacteria attributed to the DOE. Interestingly, up to 90% efficient biocidal effect is also observed for *K. pneumoniae*. The biocidal activities against Gram-positive and Gram-negative bacterial strains are encouraging and showcases the promising potential of an individual coating against a broad spectrum of bacteria.

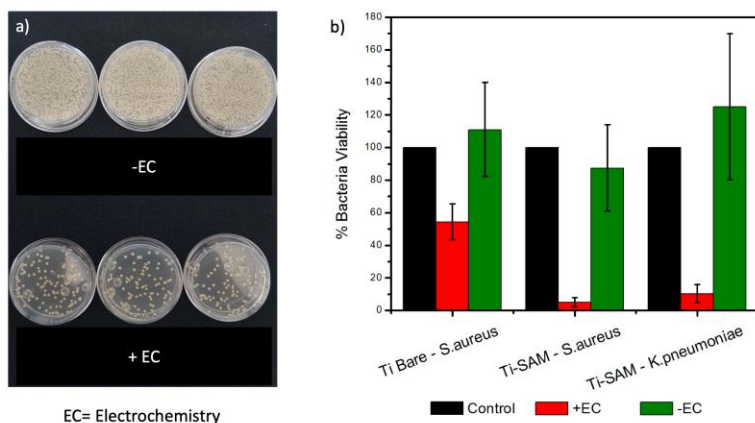

**Figure 3:** a) Petri dish captions of bacteria culture of *S. aureus* without (-EC) and with electrochemical stimuli (+EC). b) Percentage of viability of bacteria on titanium bare surface and SAM-modified Ti (3) upon contact with *S. aureus* and/or *K. pneumoniae* with (+EC) and without electrochemical (-EC) activation.

On the contrary, when no electrical step is applied, a pre-treatment of the surface was optimized to observe a full inhibition of the biocidal effect. Wherein, the molecules were forced to conformationally bend by applying a potential of -0.4V for 5 minutes before being exposed to bacteria. In this way, the bacteria viability at the interface remains close to 100%, indicating a minimal/unhesitant effect of the molecule. This pre-treatment step notably shows that it is possible to inhibit almost completely the bacteria death observing only a small loss (Figure 3). However, if the latter step is not considered the SAM-modified Ti (3) surface has a considerable action toward the bacteria death, reaching a loss equal to 70% (Figure 4). In a previous study, we have already shown that phosphonium-based ionic liquids can kill the ESKAPE group of bacterial species with low minimal inhibitory concentration (MIC), including the *S. aureus* and *K. pneumoniae* strains tested here [27]. In this case the compounds were solubilized, dispensed into the bacterial culture medium that contained  $5 \times 10^5$  CFU/mL at a final concentration, and incubated for approximately 18h, in accordance with international standard conditions for testing antimicrobial molecules (see ref 29 for details). In the present


study compound 3, an IL of the same structural basis, was self-assembled onto the titanium surface, which could strongly affect its effectiveness. Before evaluating the efficacy of SAM, the MIC of compound 3 was determined to be 3µg/mL for *S. aureus* and 16µg/mL for *K. pneumoniae*. In the experimental conditions for testing SAM, the incubation time did not exceed 60 min and the number of bacteria was about 5x10<sup>5</sup> CFU/5µL which was strongly different from MIC determination. But a current of 0.2 V was applied during the whole incubation period and, although we did not achieve the same efficiency as in the assay in liquid, we still observed a strong decrease in CFU numbers. These results demonstrated that a clever combination of an effective molecule with a weak electric field can make a SAM surface capable of hindering bacterial colonization of at least *S. aureus* and *K. pneumoniae*.

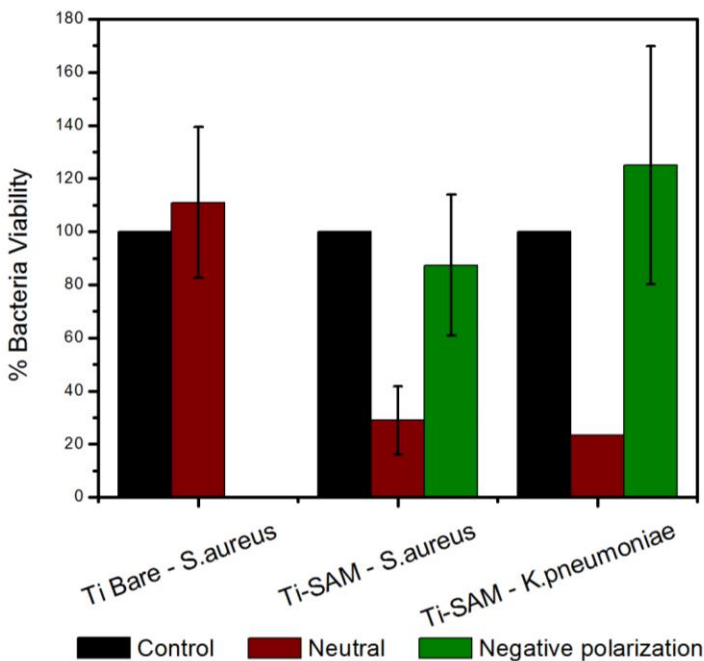

**Figure 4:** Bacteria viability of Ti bare and SAM-modified Ti (3) before (brown traces) and after negative polarization (green traces). Black traces show the control test.

In a second set of experiments, the different coatings have been tested regarding their safety towards eukaryotic cells. To conduct such experiments a novel 3D imprinted device has been designed and developed to perfectly fit on a 24 wells culture plate containing a Boyden chamber with the same diameter of the titanium disks (Figure 5a). Within this configuration the whole cell culture area is in contact with the SAM-modified titanium surfaces also avoiding a displacement of the titanium disk that could lead to the destruction of the parasitic cells hindering the real action of the modified surfaces. Furthermore, the 3D imprinted device allows the precise placement of the electrodes in height and width to the nearest mm to ensure the reproducibility of the electrochemical tests.

Fibroblast cells were selected to evaluate the biocompatibility of the coatings with and without electrical activation and compared to a control. Without electroactivation the cells viability is like the control, corroborating the non-cytotoxicity of the 3-modified titanium surfaces under these conditions. More interestingly, upon the application of the potential i.e., 0.2 V over one hour the periodontal ligament cells remain unaffected demonstrating that the electroactivation conditions are ineffective in disrupting the fibroblast cells membrane (Figure 5b).

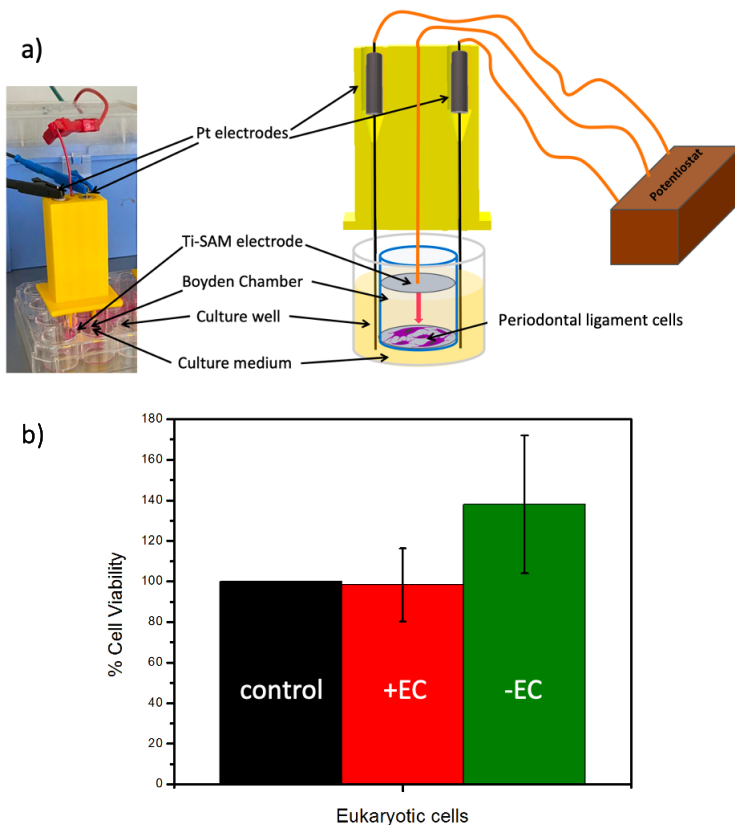

**Figure 5:** a) 3D imprinted device for the realization of the tests on eukaryotic cells. The Ti-SAM electrode is in contact with cells in the Boyden chamber, while the two Pt electrodes pass through the holes in culture well. b) % Cell viability of eukaryotic cells with and without electrochemical activation of 3-modified titanium surfaces.

## Materials and Methods

**Reagents and Materials.** 1,12-dibromododecane, 1,6-dibromohexane, tri-n-hexylphosphine, tri-n-octylphosphine, potassium thioacetate were purchased and used as received from Alfa Aesar, TCI and Sigma Aldrich. Column chromatography was performed using silica 60 M (0.04-0.063 mm) purchased from Macherey-Nagel. Solvents such as diethyl ether (Et<sub>2</sub>O), acetone, dichloromethane (DCM) were purchased from Sigma

Aldrich. Microwave irradiation experiments were conducted on a CEM Discover-SP apparatus (200W) at 130°C for 3 hours. Agarose was purchased at Invitrogen (St. Quentin Fallavier, France). Bacteria culture materials were obtained from Dominique Dutscher (Brumath, France) and the culture media were obtained from Sigma-Aldrich (Saint-Quentin Fallavier, France). The following strains were used in this study: *Staphylococcus aureus* DSM 20231 and *Klebsiella pneumoniae* DSM 102040. The strains were purchase at the Leibniz Institute DSMZ-German Collection of Microorganisms and Cell Cultures GmbH. Cell culture materials and reagents were obtained from Dominique Dutscher (Brumath, France).

Human Periodontal ligament cell Culture. Human primary periodontal ligament (hPDL) cells were prepared from immature third molars extracted for orthodontic reasons (male and female patients younger than 18 years) in compliance with French ethical legislation by the explant outgrowth method as described previously [35]. These cells were grown in minimal essential medium (MEM) supplemented with 10% fetal bovine serum, 100 U/mL penicillin, 100 mg/mL streptomycin, and 0.25 mg/mL amphotericin B at 37 °C, 5% CO<sub>2</sub> atmosphere [36].

Bacterial and cell cultures. Rehydration of dried cultures were performed as recommended by the DSMZ. All microbial strains were stored at -80°C in cryovial in Mueller-Hinton Broth II (MHII) supplemented with 30% (v/v) glycerol. Before testing, every week fresh cultures were initiated on MHII agar plate. Each day, an overnight culture was performed then a culture expansion was performed before testing.

Evaluation of interface toxicity to hPDL cells. Toxicity assays were performed in Boyden chambers. hPDL cells were plated in the upper chambers (25 000 cells in 100 µl) overnight. The Ti-SAM electrode was in contact with cells in the Boyden chamber, while the two Pt electrodes passed through the holes in culture well. According to the device configuration different conditions of electrostimulation were performed by varying the potential and duration. The medium was removed from Boyden chamber and immediately replaced with 100 µL/well MTT solution (5

mg/mL). After incubation for 2 hours at 37°C, the supernatant was discarded, and the formed formazan crystals were solubilized with dimethyl sulfoxide (Sigma-Aldrich) (300 µL/well). 100µL of each solution was transferred on 96-well dishes. Then the absorbance of each well was determined using an automatic microplate spectrophotometer (Infinite 200; Tecan, Lyon, France) at 550 nm.

Physicochemical Analysis. <sup>1</sup>H, <sup>13</sup>C and <sup>31</sup>P NMR spectra were recorded on a JEOL ECS spectrometer at 400 MHz (<sup>1</sup>H), 100 MHz (<sup>13</sup>C) or 162 MHz (<sup>31</sup>P) at room temperature. NMR chemical shifts are given in ppm (δ) relative to Me<sub>4</sub>Si with solvent resonances used as internal standards (CDCl<sub>3</sub>: 7.26 ppm for <sup>1</sup>H and 77.2 ppm for <sup>13</sup>C). <sup>31</sup>P NMR spectra are given relative to external 80% H<sub>3</sub>PO<sub>4</sub> standard. MS (ESI) analyses were performed on a SYNAPT G2 HDMS (Waters) spectrometer at the Spectropole of Aix-Marseille Université [37]. This spectrometer was equipped with an electrospray ionization source (ESI) and a Time-of-flight (TOF) mass analyzer. The sample was ionized in electrospray positive mode with a tension of 2.8 kV, the orifice tension was 50 V and the N<sub>2</sub> flow rate was 100L/h.


Contact angle measurements were performed at room temperature to access the hydrophobic/hydrophilic character of the modified substrates. Static contact angles (CA) were measured with an OCA 15 apparatus (DataPhysics) at room temperature using the sessile drop method and image analysis of the drop profile (SCA20 software). Deionized water droplet volume was 1 µl, and the contact angle was measured 10s after the drop was deposited onto the surface. Surface morphologies were conducted on untreated Ti and modified Ti using a scanning electron microscope (SEM JEOL JSM 6320F).

Physicochemical Measurements in Solution. Electrochemical studies and non-faradic impedance measurements were performed on a VersaSTAT 4 potentiostat from Princeton Applied Research (Ametek scientific instruments, France). A three-electrode system based on a titanium disk (Ti) working electrode (diameter 10 mm, thickness 0.127 mm), a platinum (Pt)

as counter and as quasi-reference electrode were used. Tetrabutylammonium hexafluorophosphate (TBAPF6) served as a supporting electrolyte (0.1 M). Titanium disks (Ti) were cut from a 99.99% pure Ti sheet from Sigma-Aldrich and subsequently polished with diamond suspension (particle sizes 5  $\mu\text{m}$ ) from ESCIL company. The freshly polished disks were subsequently rinsed and sonicated in distilled water, acetone and ethanol then followed by blow-drying with nitrogen gas under atmospheric condition. The surfaces then were exposed to a UV cleaning at 80° C for 15 minutes prior to use. Lastly, they were deep coated in a 1 mM ethanolic solution of compounds 3-5 for 2 days, to get 50% coverage or 7 days to obtain 100% coverage. The coverage percentage was monitored by using electrochemical impedance spectroscopy. Cyclic voltammetry (CV) and chronoamperometry (CA) were used as standard methods to evaluate the charge and conformational changes effects on the bacterial death. CVs were performed at a scan rate of 0.1 V/s over a potential range of +0.2V and -0.4V for 30, 60 and 120 minutes while CA's were performed at a different potential, +0.2V, +0.5V and +0.8V for 30, 60 and 120 minutes. For negative control devices, a CA at -0.4V for 5 minutes was preceding the bacterial test. Non-faradic impedance measurements were carried out at room temperature on the monolayers in the 10<sup>5</sup> to 0.05 Hz frequency range using a modulation range of 25 mV in amplitude and a dc bias of zero.

Homemade imprinted device. A device that mimics a titanium/bacteria/periodontal ligament tissue implant interface was developed by using a 3D printer (Raise 3D Pro2) from Raise 3D Technologies, Inc. The device consists of a three electrodes electrochemical cell where the Ti surface (untreated or modified) is in contact with a 1% agarose gel that mimics the gum tissue and is also used as a solid electrolyte. The other two platinum electrodes, counter, and quasi-reference have been set on the side of the device and were selected due to their robustness and low interference over the antibacterial properties. A 5  $\mu\text{L}$  bacterial suspension of *S. aureus* (strain DSM 20231) at a concentration of 10<sup>8</sup> CFU/mL was deposited between the two elements (Figure 6).



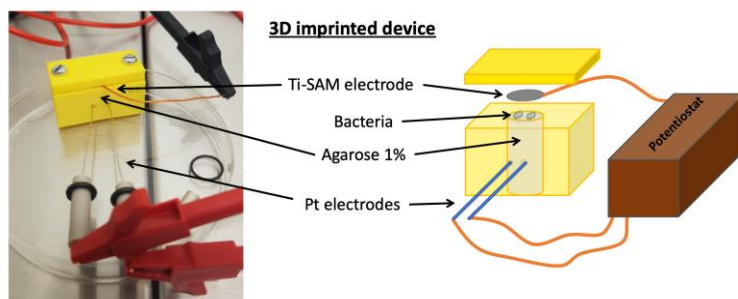

**Figure 6:** Photograph and schematic representation of the imprinted device. On the scheme the empty chamber was filled with a 1% agarose gel on which was deposited a solution of bacteria c.a.  $10^8$  CFU/mL and covered on the top by the Ti disk.

Synthesis of (12-(acetylthio)-dodecyl)-trihexylphosphonium bromide 3. In an appropriate microwave vial 2 (238 mg; 0.74 mmol; 1 eq.) and trihexylphosphine (221 mg; 0.77 mmol; 1.05 eq.) were added under inert atmosphere (glove box). Then the mixture was irradiated under microwave (200W) at 130°C for 3 hours. The obtained viscous mixture was washed, triturated and centrifuged twice with Et<sub>2</sub>O, then the supernatant was removed, and the obtained residue was taken up into DCM and dried over high vacuum. According to NMR spectrum the product was sufficiently pure to be used without further purification (449 mg; 0.73 mmol; 98% yield). <sup>1</sup>H NMR (δ, 400 MHz; CDCl<sub>3</sub>): 2.84 (t, 2H, J = 7.2 Hz), 2.44 (br, 8H), 2.3 (s, 3H), 1.42-1.58 (br, 18H), 1.21-1.36 (br, 26H), 0.88 (t, 9H, J = 6.8 Hz). <sup>13</sup>C NMR (δ, 101 MHz; CDCl<sub>3</sub>): 196.3, 31, 30.6, 29.5, 29.3, 29.2, 28.8, 22.4, 22, 19.7, 19.3, 14; 20 signals obscured or overlapping. <sup>31</sup>P NMR (δ, 162 MHz; CDCl<sub>3</sub>): 33.25. ESI MS (m/z): 529.4 (M<sup>+</sup>).

Synthesis of (12-(acetylthio)-dodecyl)-trioctylphosphonium bromide 4. In an appropriate microwave vial 2 (200 mg; 0.618 mmol; 1 eq) and trioctylphosphine (240 mg; 0.647 mmol; 1.05 eq) were added under inert atmosphere (glove box). The mixture was irradiated under microwave (200W) at 130°C for 3 hours. The obtained viscous mixture was washed with Et<sub>2</sub>O and taken up in DCM and dried over high vacuum. The product was further purified via column chromatography using DCM: MeOH (40:1) affording (210 mg; 0.342 mmol; 55 % yield) as a colorless

viscous oil. <sup>1</sup>H NMR (δ, 400 MHz; CDCl<sub>3</sub>): 2.84 (t, 2H, J= 7.3 Hz), 2.44 (br, 8H), 2.32 (s, 3H), 1.61 (br, 8H), 1.50-1.55 (m, 24H), 1.26 (br, 24H), 0.88 (t, 9H, J= 6.4 Hz). <sup>13</sup>C NMR (δ, 101 MHz; CDCl<sub>3</sub>): 196.12, 31.66, 30.84, 30.69, 29.46, 29.27, 29.05, 28.94, 28.76, 22.57, 21.93, 21.89, 19.58, 19.11, 14.05. <sup>31</sup>P NMR (δ, 162 MHz; CDCl<sub>3</sub>): 33.15. ESI MS (m/z): 613.5 (M<sup>+</sup>).

Synthesis of (6-(acetylthio)-hexyl)-trioctylphosphonium bromide 5. In an appropriate microwave vial 1 (200 mg; 0.836 mmol; 1 eq) and trioctylphosphine (309 mg; 0.833 mmol; 1.1 eq) were added under inert atmosphere (glove box). The mixture was irradiated under microwave (200W) at 130°C for 3 hours. The obtained viscous mixture was washed with Et<sub>2</sub>O and taken up in DCM and dried over high vacuum. The product was further purified via column chromatography using DCM: MeOH (40:1) to afford (190 mg; 0.358 mmol; 43 % yield) as a colorless viscous oil. <sup>1</sup>H NMR (δ, 400 MHz; CDCl<sub>3</sub>): 2.82 (t, 2H, J= 7.2 Hz), 2.46 (m, 8H), 2.31 (s, 3H), 1.71 (s, 2H), 1.45-1.56 (br, 18H), 1.31 (br, 24H), 0.87 (t, 9H, J= 6.3 Hz). <sup>13</sup>C NMR (δ, 101MHz; CDCl<sub>3</sub>): 196.02, 31.64, 30.82, 30.68, 30.63, 29.14, 28.93, 28.89, 28.69, 27.88, 22.55, 21.90, 21.86, 19.52, 19.05, 14.03. <sup>31</sup>P NMR (δ, 162 MHz; CDCl<sub>3</sub>): 33.23. ESI MS (m/z): 529.5 (M<sup>+</sup>).

## Conclusion

We reported herein the elaboration and characterization of a novel and innovative interface based on phosphonium self-assembled monolayers onto a conductive titanium surface which can be used as an effective antibacterial coating under electrical activation. The new interface possesses remarkable biocidal properties when it is electro-activated at a low potential (0.2 V) over one hour. Under these conditions, that have been determined by the help of DOE, we successfully elaborated efficient antibacterial interfaces that unambiguously kill *Staphylococcus aureus* bacteria up to 95%. Interestingly, the novel interface has also proved to be very effective in eradicating Gram-negative bacteria such as *Klebsiella pneumoniae* up to 90% under the same conditions. This unique combination of properties makes this innovative and novel interface a system of

choice for the foreseen applications. The Design Of Experiment (DOE) set up here limited considerably the number of experiments to allow us a first coverage of the study. We also considered limitation of time, to be compatible with a putative therapeutic application. In this context, while we may obtain an efficient decrease, there were still surviving bacteria, citing the need to upgrade and improve these surfaces to obtain more satisfying results. The goal must be to reach at least 99.99% of bacteria killing, and we are now considering several improvements, in particular, the development of SAMs from new molecules which are currently under study. In addition, we consider that deeper studies would be necessary to better describe the mode of action of the SAMs under an electrical field.

## References

1. Tacconelli E, Carrara E, Savoldi A, Harbarth S, Mendelson M, et al. WHO Pathogens Priority List Working Group. Discovery, research, and development of new antibiotics: the WHO priority list of antibiotic-resistant bacteria and tuberculosis, *Lancet Infect. Dis.* 2018; 18: 318-327.
2. O'Neill J. Review on antimicrobial resistance antimicrobial resistance: Tackling a crisis for the health and wealth of nations. 2014. Available online at: [https://amr-review.org/sites/default/files/AMR%20Review%20Paper%20-%20Tackling%20a%20crisis%20for%20the%20health%20and%20wealth%20of%20nations\\_1.pdf](https://amr-review.org/sites/default/files/AMR%20Review%20Paper%20-%20Tackling%20a%20crisis%20for%20the%20health%20and%20wealth%20of%20nations_1.pdf).
3. Antimicrobial resistance collaborators. Global burden of bacterial antimicrobial resistance in 2019: a systematic analysis. *Lancet.* 2022.
4. Bjarnsholt T, Jensen PØ, Moser C, Høiby N. Editors, *Biofilm infections*. New York: Springer-Verlag. 2011; 314.
5. Cattò C, Cappitelli J. Testing Anti-Biofilm Polymeric Surfaces: Where to Start? *Int. J. Mol. Sci.* 2019; 20: 1 - 60.
6. Hemmati F, Rezaee MA, Ebrahimzadeh S, Yousefi L, Nouri R, et al. Novel strategies to combat bacterial biofilms. *Mol. Biotechnol.* 2021; 63: 569-586.

7. Blackman LD, Qu Y, Cass P, Locock KES. Approaches for the inhibition and elimination of microbial biofilms using macromolecular agents. *Chem. Soc. Rev.* 2021; 50: 1587-1616.
8. Ahmed W, Zhai Z, Gao C. Adaptative antibacterial biomaterial surfaces and their applications. *Mater. Today Bio.* 2019; 100017.
9. Van Hoojs A, Van der Eeden SJF, Khatun M, Soren S, Franken KLMC, et al. BCG-induced immunity profiles in household of leprosy patients differentiate between protection and disease. *Vaccine.* 2021; 39: 7230-7237.
10. Tonkin M, Khan S, Wani MY, Ahmad A. Quorum sensing- a stratagem for conquering multi-drug resistant pathogens. *Curr. Pharm. Des.* 2021; 27: 2835-2847.
11. Borse VB, Pawar V, Shetty G, Mullaji A, Srivastava R. Nanobiotechnology perspectives on prevention and treatment of orthopaedic implant associated infection. *Curr. Drug Deliv.* 2016; 13: 175-185.
12. Kunrath MF, Campos MM. Metallic-nanoparticle release systems for biomedical implant surfaces: effectiveness and safety. *Nanotoxicology* 2021; 15: 721-739.
13. L J, Chen D, LH. Antibiofilm peptides as a promising strategy: comparative research. *Appl. Microbiol. Biotechnol.* 2021; 105: 1647-1656.
14. Li X, Wu B, Chen H, Nian K, Jin Y, et al. Recent developments in smart antibacterial surfaces to inhibit biofilm formation and bacterial infections. *J. Mater. Chem. B.* 2018; 6: 4274 - 4292.
15. Albright V, Zhuk I, Wang Y, Selin V, van de Belt Gritter B, et al. Self-defensive antibiotic-loaded layer-by-layer coatings: Imaging of localized bacterial acidification and pH-triggering of antibiotic release. *Acta Biomater.* 2017; 61: 66 - 74.
16. Ran B, Wang Z, Cai W, Ran L, Xia W, et al. Organic photo-antimicrobials: principles, molecule design, and applications. *J. Am. Chem. Soc.* 2021; 143: 17891-17909.
17. Chris Arts JJ, Geurts J. Editors, Management of periprosthetic joint infections (PJIs). United Kingdom: Woodhead Publishing Series in Biomaterials. 2017; 304.

18. Cantini E, Wang X, Koelsch P, Preece JA, Ma J, et al. Electrically responsive surfaces: experimental and theoretical investigations. *Acc. Chem. Res.* 2016; 49: 1223 - 1231.
19. Gibson JS, Wang X, Zhu Q, McGettrick JD, Watson TM, et al. On-demand electrical switching of antibody-antigen binding on surfaces. *ACS Appl. Biomater.* 2018; 1: 738 – 747.
20. Assimakopoulos D. Low intensity negative electric current in the treatment of ulcers of the leg due to chronic venous insufficiency. *Am. J. Surg.* 1968; 115: 683 – 687.
21. Rowley BA, McKenna JM, Chase GR, Wolcott LE. The influence of electrical current on an infecting microorganism in wounds. *Ann. NY Acad. of Sci.* 1974; 238: 543 - 551.
22. Del Pozo JL, Rouse MS, Patel R. Bioelectric effect and bacterial biofilms. A systematic review. *Int. J. Artif. Organs.* 2008; 31: 786 - 795.
23. Choi I, Lee J, Kim W, Kang H, Bae SW, et al. On-demand modulation of bacterial cell fates on multifunctional dynamic substrates. *ACS Appl. Mater. Interfaces.* 2018; 10: 4324 - 4332.
24. Ouyang S, Zheng K, Zhang W, Chen W, Liu Y. Microscale electric fields induced by galvanically coupled Ti-Mg metal-metal composites promote antibacterial activity. *Materials.* 2020; 9: 100621.
25. Brunel F, Lautard C, Garzino F, Giorgio S, Raimundo JM, et al. Antibacterial Activities of Fluorescent Nano Assembled Triphenylamine Phosphonium Ionic Liquids. *Bioorg. Med. Chem. Lett.* 2016; 26: 3770–3772.
26. Brunel F, Lautard C, Giorgio S, Garzino F, Raimundo JM, et al. Antibacterial Activities of mono-, di- and tri-substituted triphenylamine-based phosphoniums ionic liquids. *Bioorg. Med. Chem. Lett.* 2018; 28: 926-929.
27. Brunel F, Lautard C, Garzino F, Raimundo JM, Bolla JM, et al. Phosphonium-ammonium-based dicationic ionic liquids as antibacterial over the ESKAPE group. *Bioorg. Med. Chem. Lett.* 2020; 30: 127389.
28. Kukhta NA, Marks A, Luscombe CK. Molecular design strategies toward improvement of charges injection and ionic

- conduction in organic mixed ionic-electronic conductors for organic electrochemical transistors. *Chem. Rev.* 2021.
29. Xiong Z, Achavananthadith S, Lian S, Madden LE, Ong ZX, et al. A wireless and battery-free wound infection sensor based on DNA hydrogel. *Sci. Adv.* 2021; 7: eabj1617.
  30. Tauk L, Schröder AP, Decher G, Giuseppone N. Hierarchical functional gradients of pH-responsive self-assembled monolayers using dynamic covalent chemistry on surfaces. *Nat. Chem.* 2009; 1: 649-656.
  31. Ishfaq K, Rehman M, Khan AR, Wang Y. A review on the performance characteristics, applications, challenges and possible solutions in electron beam melted Ti-based orthopedic and orthodontic implants. *Rapid Prototyp. J.* 2021.
  32. Sidhu SS, Singh H, Gepreel MAH. A review on alloy design, biological response, and strengthening of  $\beta$ -titanium alloys as biomaterials. *Sci. Eng. C.* 2021; 121: 111661.
  33. Vizureanu P, Yamaguchi S, Le P, Baltatu M. Biocompatibility Evaluation of New TiMoSi Alloys. *Acta Phys. Pol. A* 2020; 138: 283–286.
  34. Sánchez-Bodón J, Andrade del Olmo J, Alonso JM, Moreno-Benitez I, Vilas-Vilela jL, et al. Bioactive coatings on titanium: a review on hydroxylation, self-assembled monolayers (SAMs) and surface modification strategies. *Polymers.* 2022; 14: 165.
  35. Camps J, Jeanneau C, El Ayachi I, Laurent P, About I. Bioactivity of a calcium silicate-based endodontic cement (BioRoot RCS): interactions with human periodontal ligament cells in vitro. *J. Endod.* 2015; 41: 1469-11473.
  36. Chmilewsky F, Jeanneau C, Dejoux J, About I. Source of dentin-pulp regeneration signals and their modulation by the local microenvironment, *J. Endod.* 2014; 40: S19-25.
  37. For more information, see the website of Spectropole from Aix Marseille University. Available online at: <https://fr-chimie.univ-amu.fr/spectropole/>.